

### B-ALERT WIRELESS EEG HEADSET SYSTEMS

B-Alert Wireless EEG 9-Channel System . B-ALERT110-WA

B-Alert Wireless EEG with AcqKnowledge plus Cognitive State Software . B-ALERT110-CS-WA

B-Alert Cognitive State Software . B-Alert-SFT-W (add-on software)


B-Alert Accessories, see page 3

### B-ALERT WIRELESS EEG 9-CHANNEL SYSTEM



This complete system includes the B-Alert X10 for **wireless** acquisition of 9 channels of high fidelity EEG plus ECG, head movement & position, AcqKnowledge software with powerful analysis tools, including automated scoring and reporting options, and B-Alert Cognitive State software.

- Set up in less than 5 minutes
- Comfortable and nonintrusive - low profile fits comfortably under headgear
- Data quality monitoring and feedback simplifies acquisition for non-technical personnel
- Cognitive state classification for engagement, confusion/distraction, drowsiness, workload and stress
- Patented real-time artifact decontamination

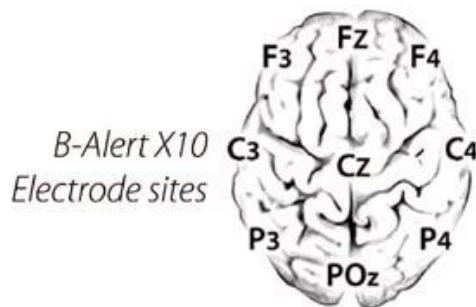

#### Standard Signals

9 mono-polar EEG with impedance  
2-lead ECG  
Heart rate  
Head movement  
PSD by channel

#### Optional signals

Differential signals for B-Alert and workload

### B-ALERT X10 WIRELESS SYSTEMS

The B-Alert X10 mobile-wireless EEG system delivers real-time measurements for a variety of research and engineering applications, including closed-loop performance monitoring and simulation training; HCI design assessment; situational awareness and team dynamics monitoring; tools for productivity and training enhancement; and fatigue management.

➡ Click to view the [B-Alert System Sample Diagram](#)


**OVERVIEW**

1. Prepare the B-Alert System.
2. Fill the foam sensors.
3. Apply X10 System to Participant.
4. Applying Mastoid and ECG Sensors.
5. Start Data Collection.
6. Remove X10 from Participant.
7. Clean X10 System.

**PLUS—CLASSIFY COGNITIVE STATES**

This system includes the B-Alert Cognitive State software with proprietary metrics for real-time monitoring of subject fatigue, stress, confusion, engagement and workload (classify data from B-Alert Wireless EEG systems). The GUI intuitively represents both the raw and processed data for easy understanding by even the untrained user and up to six systems can run simultaneously on a single PC. *Windows 10/8/7 OS only.*

To facilitate both real-time and offline analysis, the B-Alert Athena gauges are fully customizable to fit the requirements of the user. In the standard format (shown below), the easy-to-read dashboard gauges (*Top Left*) and time series (*Bottom*) windows present B-Alert's highly validated second by second metrics: Engagement, Workload and Drowsiness (along with Heart Rate). Heat maps (*Top Right*) display EEG power spectral densities (PSD) in both spatial and temporal maps for the traditional Hz bands (Beta, Alpha, Theta, Gamma).

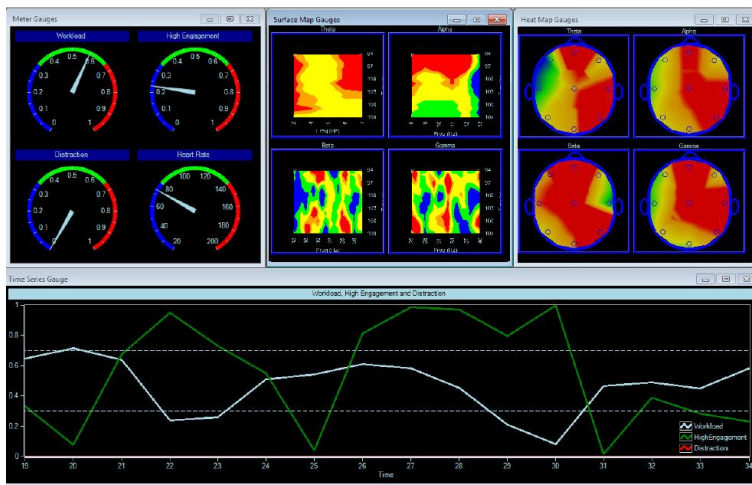

B-Alert Wireless EEG bio-metrics are normalized to an individual subject using 5-minutes of baseline data from three distinct tasks with the sleep onset class predicted from the baseline PSD values. A probability-of-fit is then generated for each of the four classes for each epoch with the sum of the probabilities across the four classes equaling 1.0 (e.g., 0.45 high engagement, 0.30 low engagement, 0.20 distraction and 0.05 sleep onset). Cognitive State for a given second represents the class with the greatest probability. B-Alert cognitive state metrics are derived for each one-second epoch using 1 Hz power spectra densities (PSD) bins from differential sites FzPO and CzPO in a four-class quadratic discriminant function analysis (DFA) that is fitted to the individual's unique EEG patterns. The table briefly describes each baseline task and the B-Alert classification.

Baseline task	Action	B-Alert Class probabilities
3-choice vigilance task (~7-min; optional 20-min)	Choose between primary vs. secondary or tertiary task every 1.5 to 3-seconds	High Engagement
Eyes open (5-min)	Respond to visual probe every 2-seconds	Low Engagement
Eyes closed (5-min)	Respond to audio tone every 2-seconds	Distraction if episodic Drowsy if sequential
None	Derived by regression from other three tasks	Sleep Onset

**B-ALERT COGNITIVE STATE SOFTWARE (ADD-ON, SOFTWARE ONLY)**

Classify Cognitive States with this analysis software add-on for B-Alert Systems (Windows 10/8/7 OS only)

**B-ALERT ACCESSORIES**

**Disposable Study Kits**

**RXB-ALERT-KIT-S or RXB-ALERTKITA-S**

small 32.0-34.5 cm (approx. 12.6-13.6")

**RXB-ALERT-KIT-M or RXB-ALERTKITA-M**


medium > 34.5 cm

Each disposable study kit for the B-Alert X10 Wireless EEG System contains:

- one sensor strip
- foam sensors
- one Neoprene sensor strap with Velcro
- disposable electrodes (for mastoid) for 25 studies
- gel and pads for 25 studies



Order kit based on size and B-Alert headset style:

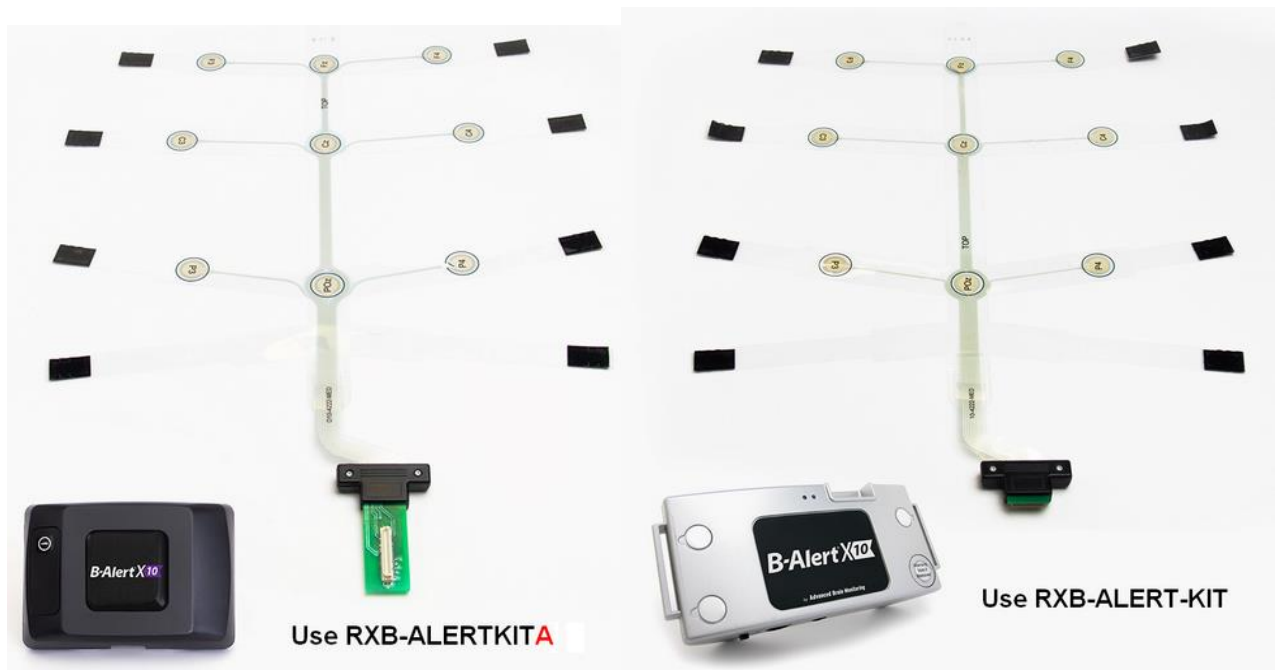

**HARDWARE SPECIFICATIONS:**

Channels:	9 EEG with fixed gain referenced to linked mastoids; 1 auxiliary differential channel with programmable gain
Sampling rate:	256 samples/second . all channels
Dynamic range:	+/- ± 1,000-2000 $\mu$ V
Resolution:	16 bit, CMRR 105 dB
Input impedance:	500 M $\Omega$ , typical
Common mode rejection ratio:	-115 dB, typical
Bandpass characteristics:	0.1 Hz HPF Firmware, and 67 Hz LPF hardware
Noise:	3 $\mu$ V peak-to-peak typical
Head movement/position:	Angles obtained with 3-axis 12-bit accelerometer
RF Band:	Bluetooth 2.4 to 2.48 GHz (ISM band), latency < 340 ms
Transmission mode:	Bluetooth SPP 2.0 via USB dongle or external synching unit
Data transmission range:	~ 10 meters, line of sight with onboard antenna
Transmission power:	Class 2 +4 dBm
System power consumption:	~ 60 mAh
Battery capacity:	Standard 2 x Li-ION batteries - 600 mAh, 11-hours of continuous use
Battery charging:	Via USB cable connected to USB port or USB wall charger
On-line impedance monitoring:	Initiated by host computer using Bluetooth
Head unit dimensions:	Size 6.83 cm (L) x 4.83 cm (W) x 2.03 cm (H); Weight 57 g
User control:	On/Off
Indicator LEDs:	Green/Amber
Software Compatibility:	Windows 10, 8 and 7, PC with 2.0 GHz or higher processor 1 GB of RAM
<b>Sensor Headset &amp; Accessories</b>	
Sensor sites:	Referential: Fz, F3, F4, Cz, C3, C4, POz, P3, P4
Sensor strip sizes:	X-small, Small, & Medium . each site $\pm$ 1 cm of 10-20 system Medium = Nasion to Inion ~36 cm
Electrode cream:	Highly conductive, electrolytes and preservatives in hypoallergenic base, buffered to skin pH